

Validation Report #029597

Validation Date: 02/09/14

Summary

Antigen	human Epidermal Growth Factor Receptor (EGFR)
Catalog number	ABIN837930
Supplier	Cusabio
Supplier catalog number	CSB-E12124h
Lot number	S24095908
Method validated	Enzyme-linked immunosorbent assay
Laboratory	Alamo Laboratories Inc
Validation number	29597
Positive Control	Human individual postmenopausal female serum
Negative Control	Goat serum
Notes	Signal was detected in the positive control sample and not in the negative control sample.



Full Methods

Primary Antibody

- Antigen: Human epidermal growth factor receptor, EGFR
- Catalog Number: ABIN837930
- Supplier: Cusabio
- Supplier catalog number: CSB-E12124h
- Lot Number: S24095908

Controls

- Positive control: Serum from normal adult human (specimen known to contain the target protein).
- Negative control: Serum from normal goat (specimens known to not contain the target protein).
- Standard curve: Serial two-fold dilutions from 20 ng/ml [20, 10, 5, 2.5, 1.25, 0.625, 0.312, 0] were generated from the standard provided in the kit using standard/sample diluent buffer.
- Spike control: Standard diluted in standard/PBS diluent buffer [1.25 and 0].

Protocol

- All reagents in the ELISA kit were brought up to room temperature (RT) before use.
- 100 μ L of standard or sample were added to wells in ELISA plate pre-coated with capture antibody. All samples and standards were assayed in triplicate.
- The plate was covered with sealer (provided in kit) and incubated for 2 hours at 37°C. Unbound material was aspirated but the wells were NOT Washed.
- 100 μ L of Biotin-Antibody (diluted 1:100 in "Biotin-Antibody Diluent") was added to each well. Plate was covered with sealer (provided in kit) and incubated for 1 hour at 37°C. Unbound Biotin-Antibody was removed from each well and plate was washed three times with 350 μ L of wash buffer (provided in the kit). After the last wash the plate was inverted against clean absorbent paper to remove any remaining liquid.
- 100 μ L of HRP-Avidin Conjugate (diluted 1:100 in "HRP-Avidin Diluent") was added to each well. Plate was covered with sealer (provided in kit) and incubated for 1 hour at 37°C.
- Unbound HRP-Avidin was removed by washing five times with 350 μ L of wash buffer (provided in the kit). After the last wash the plate was inverted and blotted against clean absorbent paper to remove any remaining liquid.
- 90 μ L of TMB substrate was added to wells and the plate was covered with a new plate sealer. The plate was gently tapped to ensure mixing and incubated for 30 min at 37°C in the dark.
- After 30 min, when an apparent gradient appeared in the standard wells, the reaction was terminated by adding 50 μ L of Stop Solution to each well.
- The optical density (OD value) of each well was read using a microplate reader set to 450 nm.
- The triplicate readings for each sample were averaged and the average zero standard optical density subtracted to yield 'corrected absorbance at 450 nm'. A standard curve was generated by plotting the mean OD value for each standard on the X-axis against the concentration on the Y-axis using Excel. Standard curve was generated by regression analysis with four-parameter logistic.
- An equation ($y = 12.72x^4 - 22.038x^3 + 16.56x^2 + 8.1457x$) was derived from the standard curve and used to calculate Epidermal Growth Factor Receptor concentrations in samples based on their Average Absorbance values.

Experimental Notes

None

Figures

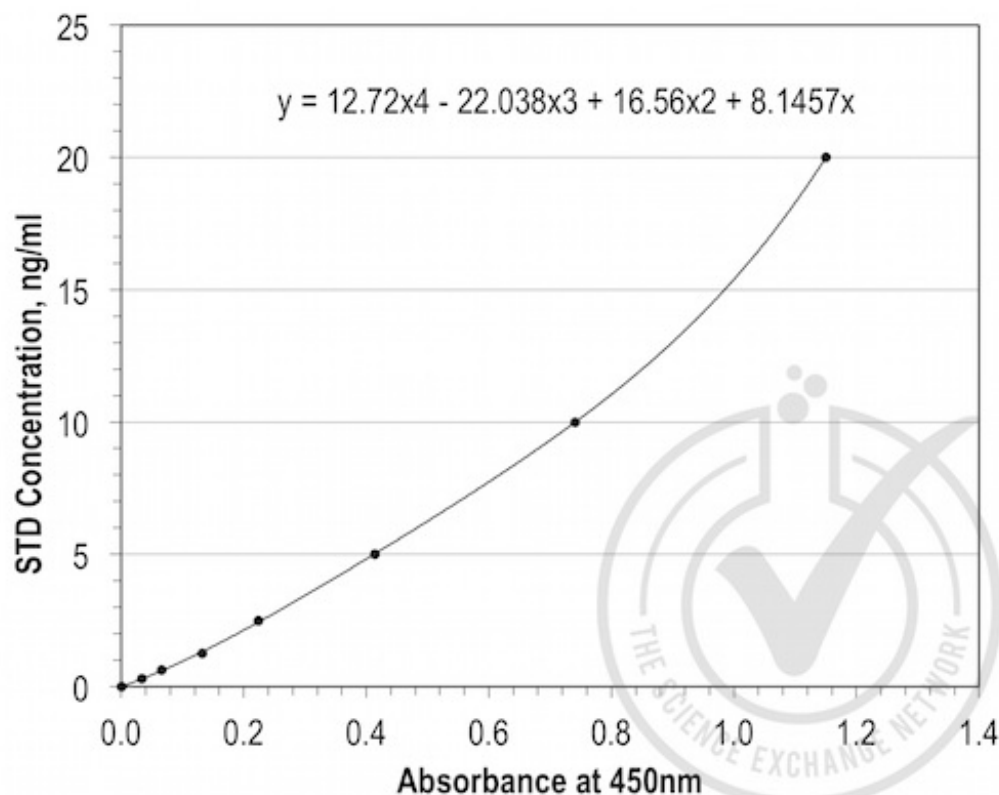


Figure 1: Graph of corrected OD450 nm plotted for standard curve samples.

Type	Sample, ng/ml	Readings at 450 nm			Avg Reading	Corrected OD _{450nm}	SD	Calculated conc ng/ml
		1	2	3				
Standards	20	1.256	1.209	1.207	1.224	1.150	0.023	20.00
	10	0.819	0.813	0.813	0.815	0.741	0.003	10.00
	5	0.476	0.498	0.489	0.488	0.414	0.009	5.02
	2.5	0.308	0.274	0.313	0.298	0.224	0.017	2.44
	1.25	0.207	0.206	0.206	0.206	0.132	0.000	1.32
	0.625	0.138	0.136	0.146	0.140	0.066	0.004	0.60
	0.312	0.108	0.110	0.107	0.108	0.034	0.001	0.30
	0	0.082	0.070	0.071	0.074	0.000	0.005	0.00
Spike Controls	1.25	0.198	0.222	0.189	0.203	0.130	0.014	1.29
	0.00	0.068	0.074	0.076	0.073	0.000	0.003	0.00
Test Samples	Serum, Woman, 73Yr	1.445	1.308	1.371	1.375	1.302	0.056	26.57
	Serum, 1:10 Dil Woman, 73Yr	0.638	0.624	0.646	0.636	0.563	0.009	7.18
	Serum, Goat	0.069	0.070	0.076	0.072	-0.001	0.003	-0.01

EGFR conc in 1:10 Diluted Serum, woman73Yr (+ve Control): 7.18×10 (dilu factor) = 71.8 ng/ml.

EGFR conc in undiluted Serum, woman73Yr (+ve Control): 26.57 ng/ml *Out-of-range of STD curve*.

EGFR conc in Goat Serum (-ve Control) : - 0.01 ng/ml

Table 1: ELISA. Epidermal Growth Factor Receptor is present in human serum and undetectable in goat serum. Spike controls indicate no interference in absorbance readings from the diluent used to prepare standards and sera samples. Absorbance readings (OD450 nm) are shown for standard curve, spike controls and unknown samples.

Value for Avg Reading is derived from the average reading of three samples. Avg Reading for "0" amount of Standard was subtracted from all Avg Readings to yield "Corrected OD450 nm" values for Standards, spike controls and unknown samples. Standard deviation is included for all samples. Standard curve was generated by regression analysis with four-parameter logistic. An equation ($y = 12.72x^4 - 22.038x^3 + 16.56x^2 + 8.1457x$) was derived from the standard curve and used to calculate Epidermal Growth Factor Receptor concentrations shown in Table 1.