



Datasheet for ABIN6963346

Insulin ELISA Kit



[Go to Product page](#)

1 Image

3 Publications

Overview

Quantity:	96 tests
Target:	Insulin (INS)
Reactivity:	Rat
Method Type:	Sandwich ELISA
Detection Range:	6.25 pg/mL - 400 pg/mL
Minimum Detection Limit:	6.25 pg/mL
Application:	ELISA

Product Details

Purpose:	The kit is a sandwich enzyme immunoassay technique for the in vitro quantitative measurement in various sample types.
Sample Type:	Cell Culture Supernatant, Plasma, Serum
Analytical Method:	Quantitative
Detection Method:	Colorimetric
Specificity:	This kit recognizes Rat INS in samples. No significant cross-reactivity or interference between Rat INS and analogues was observed.
Sensitivity:	3.75 pg/mL
Components:	<ul style="list-style-type: none">• Pre-coated, ready to use 96-well strip plate, flat bottom• Plate sealer for 96 wells• Reference Standard• Reference Standard & Sample Diluent

Product Details

- Biotinylated Detection Antibody (100 x concentrate)
- HRP Conjugate (100 x concentrate)
- Biotinylated Detection Antibody Diluent
- HRP Conjugate Diluent
- Substrate Reagent
- Stop Solution
- Wash Buffer (25 x concentrate)
- Instruction manual

Target Details

Target:	Insulin (INS)
Alternative Name:	Insulin (INS Products)
Background:	IDDM2, ILPR, IRDN, MODY10
Pathways:	NF-kappaB Signaling , RTK Signaling , Positive Regulation of Peptide Hormone Secretion , Peptide Hormone Metabolism , Hormone Activity , Carbohydrate Homeostasis , ER-Nucleus Signaling , Regulation of Carbohydrate Metabolic Process , Feeding Behaviour , Autophagy , Negative Regulation of intrinsic apoptotic Signaling , Brown Fat Cell Differentiation , Positive Regulation of fat Cell Differentiation

Application Details

Sample Volume:	100 µL
Assay Time:	3.5 h
Plate:	Pre-coated
Protocol:	<ol style="list-style-type: none">1. Add 100 µL standard or sample to each well. Incubate for 90 min at 37 °C.2. Remove the liquid. Add 100 µL Biotinylated Detection Antibody. Incubate for 1 hour at 37 °C.3. Aspirate and wash 3 times.4. Add 100 µL HRP Conjugate. Incubate for 30 min at 37 °C.5. Aspirate and wash 5 times.6. Add 90 µL Substrate Reagent. Incubate for 15 min at 37 °C.7. Add 50 µL Stop Solution. Read at 450 nm immediately.8. Calculation of results.
Reagent Preparation:	<ol style="list-style-type: none">1. Bring all reagents to room temperature (18-25 °C) before use. If the kit will not be used up in one assay, please only take out the necessary strips and reagents for present experiment, and store the remaining strips and reagents at required condition.2. Wash Buffer: Dilute 30 mL of Concentrated Wash Buffer with 720 mL of deionized or distilled

- water to prepare 750 mL of Wash Buffer. Note: if crystals have formed in the concentrate, warm it in a 40 °C water bath and mix it gently until the crystals have completely dissolved.
3. Standard working solution: Centrifuge the standard at 10,000xg for 1 min. Add 1.0 mL of Reference Standard & Sample Diluent, let it stand for 10 min and invert it gently several times. After it dissolves fully, mix it thoroughly with a pipette. This reconstitution produces a working solution of 400pg/mL (or add 1.0 mL of Reference Standard & Sample Diluent, let it stand for 1-2 min and then mix it thoroughly with a vortex meter of low speed. Bubbles generated during vortex could be removed by centrifuging at a relatively low speed). Then make serial dilutions as needed. The recommended dilution gradient is as follows: 400, 200, 100, 50, 25, 12.5, 6.25, 0pg/mL. Dilution method: Take 7 EP tubes, add 500µL of Reference Standard & Sample Diluent to each tube. Pipette 500µL of the 400pg/mL working solution to the first tube and mix up to produce a 200pg/mL working solution. Pipette 500µL of the solution from the former tube into the latter one according to this step. The illustration below is for reference. Note: the last tube is regarded as a blank. Don't pipette solution into it from the former tube.
 4. Biotinylated Detection Antibody working solution: Calculate the required amount before the experiment (100 µL/well). In preparation, slightly more than calculated should be prepared. Centrifuge the Concentrated Biotinylated Detection Antibody at 800xg for 1 min, then dilute the 100x Concentrated Biotinylated Detection Antibody to 1x working solution with Biotinylated Detection Antibody Diluent (Concentrated Biotinylated Detection Antibody: Biotinylated Detection Antibody Diluent = 1: 99).
 5. HRP Conjugate working solution: Calculate the required amount before the experiment (100 µL/well). In preparation, slightly more than calculated should be prepared. Centrifuge the Concentrated HRP Conjugate at 800xg for 1 min, then dilute -6- the 100x Concentrated HRP Conjugate to 1x working solution with HRP Conjugate Diluent (Concentrated HRP Conjugate: HRP Conjugate Diluent = 1: 99). 400 200 100 50 25 12.5 6.25 0

Sample Preparation:

- It is recommended to use fresh samples without long storage, otherwise protein degradation and denaturation may occur in these samples, leading to false results. Samples should therefore be stored for a short period at 2 - 8 °C or aliquoted at -20 °C (≤1 month) or -80 °C (≤3 months). Repeated freeze-thaw cycles should be avoided. Prior to assay, the frozen samples should be slowly thawed and centrifuged to remove precipitates.
- If the sample type is not specified in the instructions, a preliminary test is necessary to determine compatibility with the kit.
- If a lysis buffer is used to prepare tissue homogenates or cell culture supernatant, there is a possibility of causing a deviation due to the introduced chemical substance. The recommended dilution factor is for reference only.
- Please estimate the concentration of the samples before performing the test. If the values are not in the range of the standard curve, the optimal sample dilution for the particular experiment has to be determined. Samples should then be diluted with PBS (pH = 7.0-7.2).

Assay Precision:

Intra-assay Precision (Precision within an assay): 3 samples with low, mid range and high level Rat INS were tested 20 times on one plate, respectively.

Inter-assay Precision (Precision between assays): 3 samples with low, mid range and high level

Application Details

Rat INS were tested on 3 different plates, 20 replicates in each plate.

Both intra-CV and inter-CV are < 10 %.

Restrictions: For Research Use only

Handling

Storage: 4 °C,-20 °C

Storage Comment:

1. For unopened kit: All reagents should be stored according to the labels on the vials, so they are stable up to 6 months after receipt of the kit. The Reference Standard, Biotinylated Detection Antibody, HRP Conjugate and the 96-well stripe plate should be stored at -20 °C upon receipt while the other reagents should be stored at 4 °C.
2. For used kit: When the kit is used, the remaining reagents need to be stored according to the above storage condition. Besides, please return the unused wells to the foil pouch containing the desiccant pack, and zip-seal the foil pouch.

Expiry Date: 6 months

Publications

Product cited in: Al-Hakeim, Najm, Al-Dujaili, Maes: "Major Depression in Children with Transfusion-Dependent Thalassemia Is Strongly Associated with the Combined Effects of Blood Transfusion Rate, Iron Overload, and Increased Pro-inflammatory Cytokines." in: **Neurotoxicity research**, Vol. 38, Issue 1, pp. 228-241, (2021) ([PubMed](#)).


Kilanczyk, Banales, Wunsch, Barbier, Avila, Mato, Milkiewicz, Milkiewicz: "S-adenosyl-L-methionine (SAME) halts the autoimmune response in patients with primary biliary cholangitis (PBC) via antioxidant and S-glutathionylation processes in cholangiocytes." in: **Biochimica et biophysica acta. Molecular basis of disease**, Vol. 1866, Issue 11, pp. 165895, (2020) ([PubMed](#)).

Atwany, Hashemi, Jayakumar, Nagarkatti, Nagarkatti, Hassuneh: "Induction of CD4+CD25+ Regulatory T Cells from In Vitro Grown Human Mononuclear Cells by Sparteine Sulfate and Harpagoside." in: **Biology**, Vol. 9, Issue 8, (2020) ([PubMed](#)).

Liu, Wang, Song, Sun, Hong, Pothukuchi, Xu: "Systematically transplanted human gingiva-derived mesenchymal stem cells regulate lipid metabolism and inflammation in hyperlipidemic mice with periodontitis." in: **Experimental and therapeutic medicine**, Vol. 19, Issue 1, pp. 672-682, (2020) ([PubMed](#)).

Zheng, Sun, Xu, Pan, Zhang, Fang, Fang, Cai: "Clinical characteristics of 34 COVID-19 patients admitted to intensive care unit in Hangzhou, China." in: **Journal of Zhejiang University. Science. B**, Vol. 21, Issue 5, pp. 378-387, (2020) ([PubMed](#)).

Images

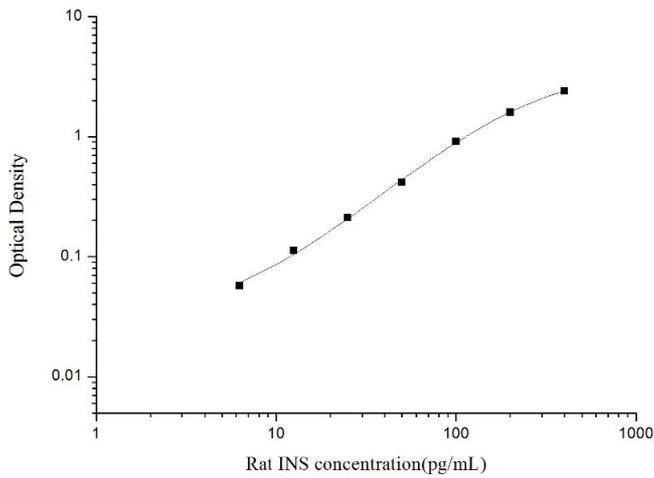

ELISA

Image 1. Typical standard curve